



TOR CDR

CONVENTIONAL AND DIGITAL RADIOGRAPHY

A routine test object designed to be used quickly and easily on a regular basis (e.g. weekly or monthly) to provide an ongoing check of imaging performance, particularly those aspects which are most liable to deterioration. After an initial grey-scale check, image quality is measured simply by counting the number of details detected and the number of bar-patterns resolved in the image. An ongoing record of these numbers will reveal any trend towards deterioration in imaging performance.

Used for conventional and non-subtractive digital radiography, enables the following checks to be made:

Sensitometric measurements
(10 test point details, 5.6mm diameter)

Resolution limit
(0.5 to 14.3 LP/mm)

Low-contrast large-detail detectability
(17 details, 11mm diameter, contrast range 0.002 to 0.075 @ 70kVp 1mm Cu)

High-contrast small-detail detectability
(17 details, 0.5mm diameter, contrast range 0.039 to 0.954 @ 70kVp 1mm Cu)

In addition to checking the consistency of radiographic performance, the test object can be used to assess the relative performance of different screen-film combinations.




For more information or to find your regional distributor please visit our website

www.leadstestobjects.com | tel. +44(0)1423 321102



TOR CDR

CONVENTIONAL AND DIGITAL RADIOGRAPHY

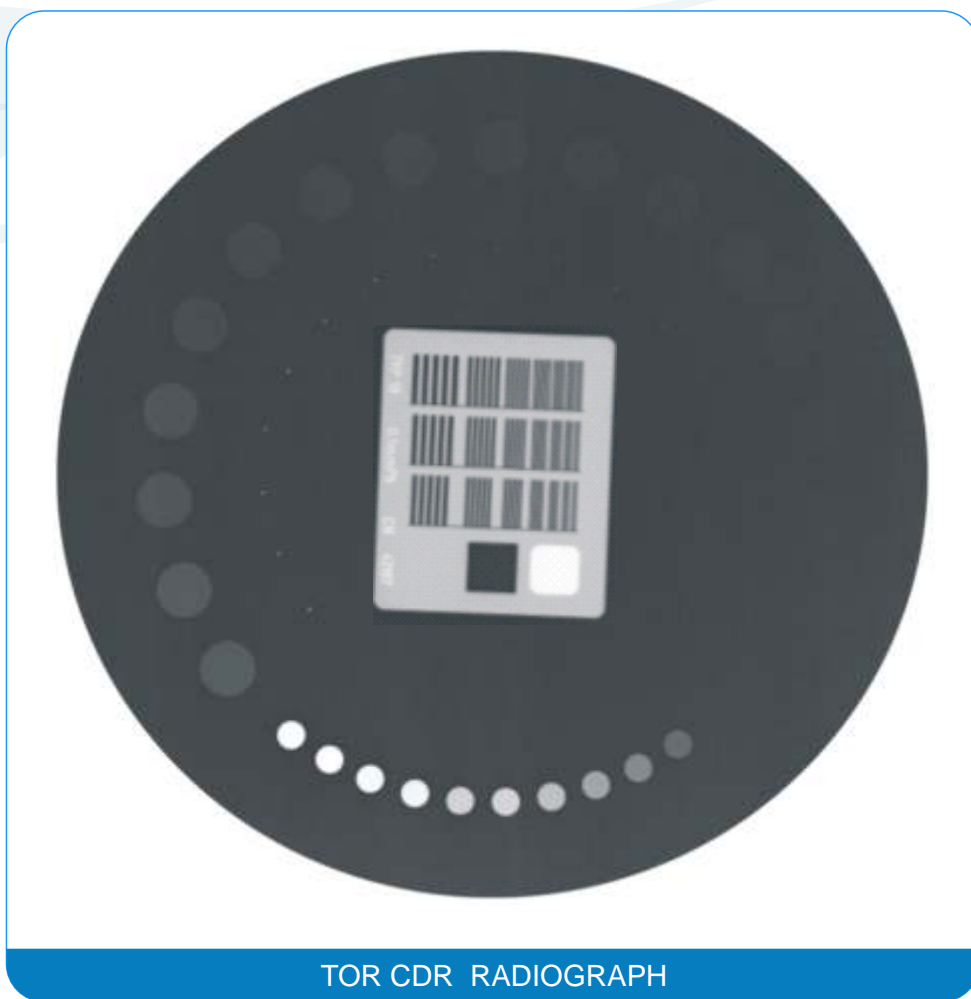

TOR CDR RADIOGRAPH

For more information or to find your regional distributor please visit our website

www.leadstestobjects.com | tel. +44(0)1423 321102

Copyright © 2011 Leeds Test Objects Ltd | SpecSh 175b 16/02/2012